


SPECTRUM DATA

OPTIMA Didymium Filter

DATE : Feb. 01. 2005

Wavelength(nm)	352	432	474	514	532	574	586	686	740	808	880
Transmissivity(%)	14.41	63.47	68.65	44.77	29.76	1.45	1.02	72.80	7.94	3.80	34.41
Absorbance	0.841	0.197	0.163	0.349	0.526	1.839	1.990	0.138	1.100	1.420	0.463

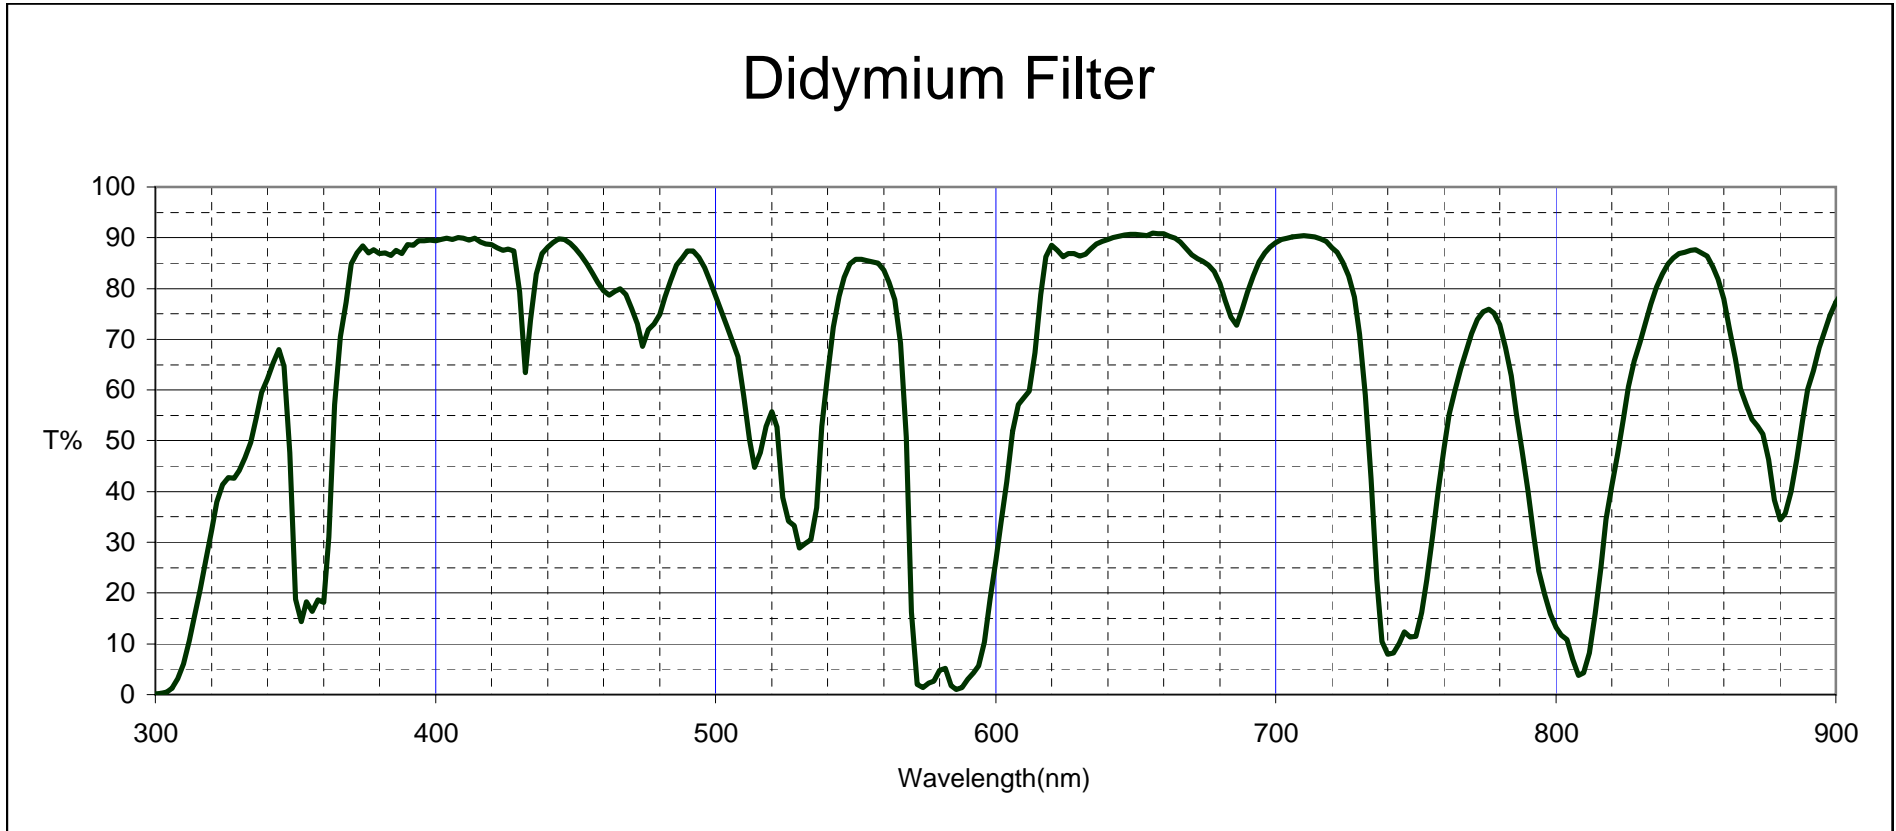

Color Glass Filter (OPTIMA INC. JAPAN)

- 1) Model : OPTIMA Didymium Filter
- 2) Test Instrument : SP-3000 Plus
- 3) Scan Interval : 2 nm
- 4) Part No.: 30008 & 30009

Inspector : Technomart Inc. Eng. Div.

SEO, IL-SOO